

We Image Your Needs.



* Cor
Cam™




Gamma camera system
for nuclear cardiology procedures




Toll Free: 888-239-3510 | Fax: 636-239-6221
207 Lange Drive | Washington, MO 63090
www.uni-med.com

* Pending 510k approval



**Cor
Cam™**

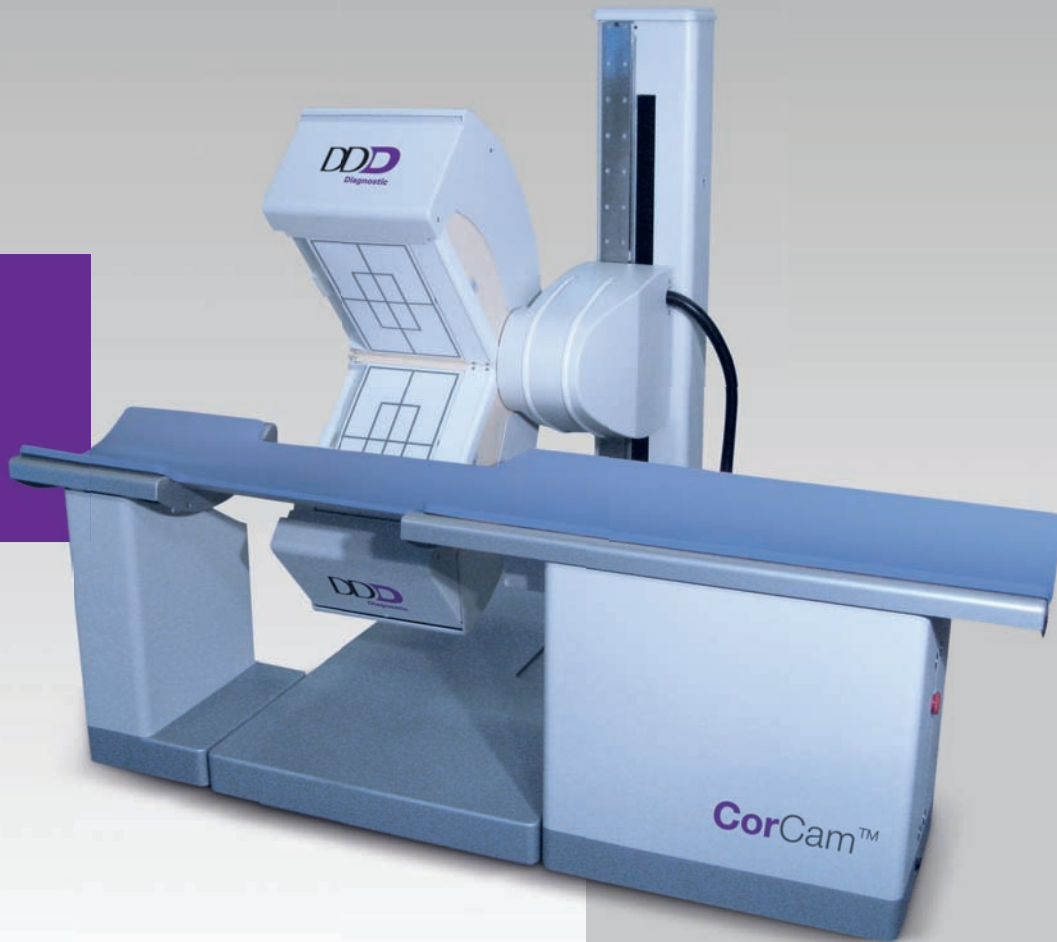

**Optimized for quick
and seamless
Myocardial Perfusion
Imaging.**

**Highly reliable and well proven
gamma camera.**

**Truly open gantry allows for
greater patient comfort.**

**Integrates with hospital
infrastructure –
DICOM Modality Work List.**

Available in two version

- 1) Supine imaging with minimal footprint.
- 2) Supine and prone imaging with small footprint.



DDD is the leading manufacturer of gamma cameras for Myocardial Perfusion Imaging.

Thousands gamma camera systems manufactured by **DDD-Diagnostic A/S** have been installed in hospitals, private practices and imaging centers across the world.

Like the other camera systems from **DDD-Diagnostic A/S**, **CorCam™** has been designed as a workhorse camera for nuclear cardiology imaging procedures.



Main Specifications

CorCam™
Type No. 9COR2370

Detector Performance	
UFOV	36 × 20.4 cm (37 × 21.4 cm imaged FOV)
Energy range	55–200 keV
Intrinsic spatial resolution (UFOV)	<3.8 mm (FWHM), <7.6 mm (FWTM)
Intrinsic spatial linearity (UFOV)	<0.2 mm (Differential), <0.5 mm (Absolute)
Intrinsic energy resolution (UFOV)	<9.4 %
Intrinsic flood field uniformity (UFOV)	<1.5 % (Differential), <2.5 % (Integral)
Intrinsic count rate performance wo. Scatter	200 kcps
Collimators	LEHR and LEGP
System Performance	
System spatial resolution wo. Scatter	
LEHR (140 keV)	<7.7 mm FWHM @ 100 mm
LEGP (140 keV)	<9.4 mm FWHM @ 100 mm
System planar sensitivity	
LEHR (140 keV)	191 cpm μ Ci +/- 7%
LEGP (140 keV)	277 cpm μ Ci +/- 7%
Detector-detector sensitivity variation	5%
Center of rotation error	<4.6 mm _{pp}
Image acquisition	
Supported imaging procedures	Static, dynamic, gated planar, SPECT and gated SPECT
Pixel size	6.4 mm square (64 matrix). 1–5 zoom
Matrix size	64 × 64, 128 × 128, 256 × 256, 512 × 512 pixels
DICOM	DICOM 3.0. Manual and automatic “push” protocol to user-provided nuclear medicine workstation. DICOM Modality Work List as an option.
General	
Power requirement	100–120 VAC, 200–240 VAC. 50/60Hz
Weight	<1,000 kg (<2204 lbs.)
Minimum room size requirement	
• Version for supine imaging	2.45 × 3.05 m (8' × 10")
• Version for supine and prone imaging	3.35 × 3.05 m (10,9' × 10")
Table Load Limit	180 kg (400 lbs.)

[DATA SUBJECT TO CHANGE]



**CorCam™ is designed,
developed and manufactured
by DDD-Diagnostic A/S in Denmark.**

DDD is a well known OEM manufacturer of gamma camera systems. Early 2012 the first products under own brand were also released to the market.

DDD was founded in 1987 and has been involved in design and development of some of the most successful gamma camera systems in cooperation with major international vendors of medical diagnostic imaging equipment.



Toll Free: 888-239-3510
Fax: 636-239-6221
207 Lange Drive
Washington, MO 63090
www.uni-med.com